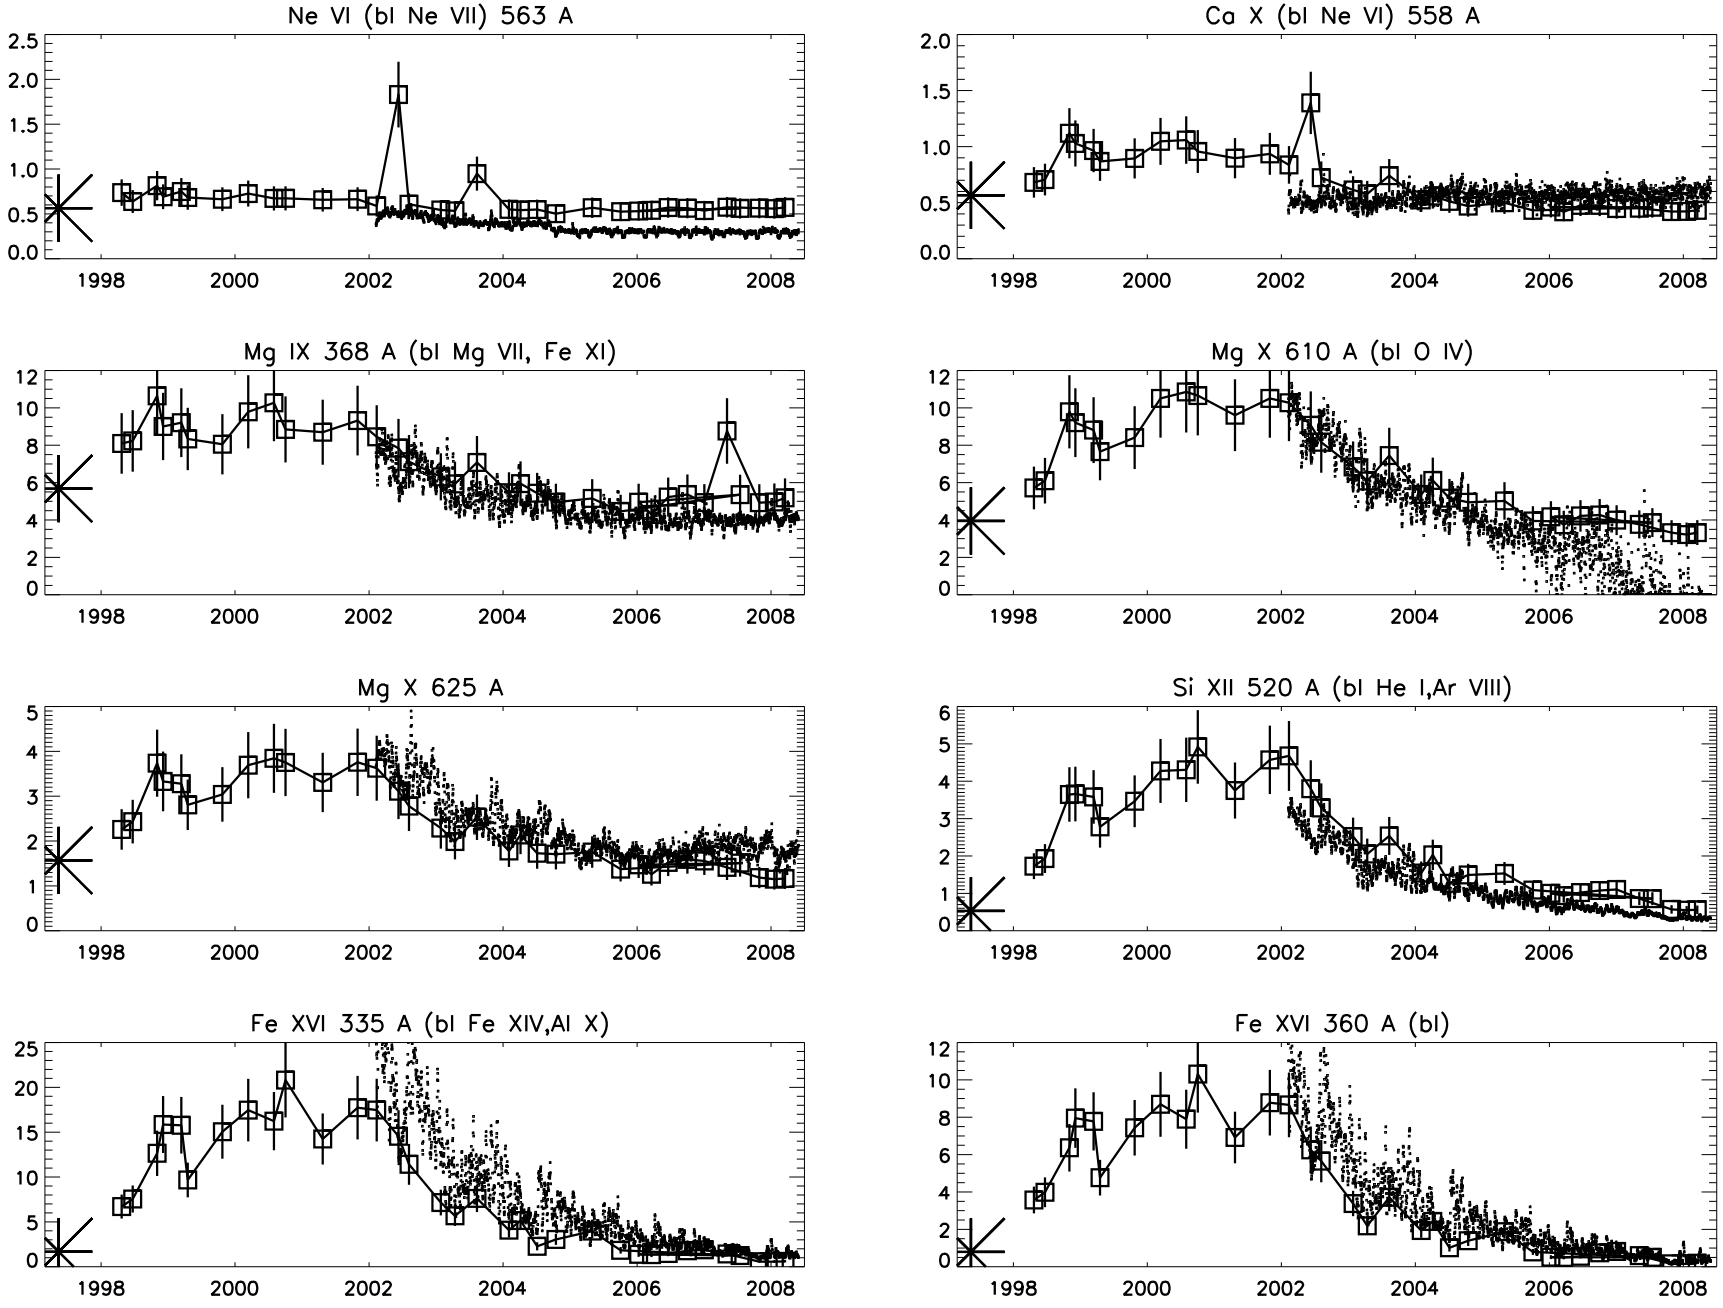CDS Irradiances – Standard calibration – standard slit 6 correction